

CERTIFICATE OF CALIBRATION

ISSUED BY: INSTRON CALIBRATION LABORATORY

DATE OF ISSUE: 21-Aug-14

CERTIFICATE NUMBER: 22082114091500



Instron

825 University Avenue

Norwood, MA 02062-2643

Telephone: (800) 473-7838

Fax: (781) 575-5750

Email: service_requests@instron.com

Page 1 of 5 pages

APPROVED SIGNATORY

Walt
Szymanowski

Digitally signed by Walt Szymanowski
DN: cn=Walt Szymanowski, o=US, ou=Norwood,
st=MA, ou=Instron, ou=America's - MARK Calibration
Laboratory, A Division of Instron Test Works, Inc. (ITW,
Inc.), email=Walt_Szymanowski@instron.com
Date: 2014.08.21 11:21:21 -0400

Type of Calibration: Force
Relevant Standard: ASTM E4-13
Date of Calibration: 21-Aug-14

Customer Requested Due Date: 21-Feb-16

Customer

Name: US Army Rodman Test Center
Address: Bldg. 4600
Aberdeen Proving Grounds, Md. 21005

P.O./Contract No.:

Contact:

Machine

Manufacturer: Instron
Serial Number: 5500R1125 / 6677
System ID: 5500R1125 / 6677
Range Type: Single

Transducer

Manufacturer: Instron
Transducer ID: 2511-325 / 374
Capacity: 5620 lbf
Type: Tension/Compression

Classification

I. Service Port - PASSED

Certification Statement

This certifies that the forces verified with machine indicator(s) (listed above) that passed are WITHIN $\pm 1\%$ accuracy, 1% repeatability, and zero return tolerance.

All machine indicators were verified on-site at customer location by Instron in accordance with ASTM E4.

The certification is based on runs 1 and 2 only. A third run is taken to satisfy uncertainty requirements according to ISO 17025 specifications.

The verification and equipment used conform to a controlled Quality Assurance program which meets the specifications outlined in ANSI/NCSL Z540-1, ISO 10012, ISO 9001:2008 and ISO/IEC 17025:2005.

Method

The testing machine was verified in the 'as found' condition with no adjustments carried out.

Instron CalproCR Version 3.27

The results indicated on this certificate and the following report relate only to the items verified. If there are methods or data included that are not covered by the NVLAP accreditation it will be identified in the comments. Any limitations of use as a result of this verification will be indicated in the comments. This report must not be used to claim product endorsement by NVLAP or the United States government. This report shall not be reproduced, except in full, without the approval of the issuing laboratory.

CERTIFICATE OF CALIBRATION

NVLAP ACCREDITED CALIBRATION LABORATORY No. 200301-0

CERTIFICATE NUMBER:

22082114091500

Page 2 of 5 pages

Summary of Results

Temperature at start of verification: 64.90 °F.

Indicator 1. - Service Port (lbf)

Range	Tested Force Range	Mode	ASTM E4 Max Error (%)	ASTM E4 Max Repeat Error (%)	Zero Return	Resolution (lbf)	ASTM E4 Lower Limit (lbf)
Full Scale (%)	(lbf)						
100	111.9768 to 4974.9	T	0.55	0.16	Pass	0.0562	11.24
	-118.8512 to -4981.1	C	0.37	0.09	Pass	0.0562	11.24

Temperature at end of verification: 64.90 °F.

Data Point Summary - Indicator 1. - Service Port (lbf)

TENSION

% of Range	Run 1 Error (%)	Run 2 Error (%)	Run 3 Error (%)	ASTM E4 Repeat Error (%)	Relative Uncertainty*	Uncertainty of Measurement* (± lbf)
100% Range (Full Scale: 4974.9 lbf)						
2	0.13	0.09	0.42	0.04	0.25	0.28
4	0.16	0.23	0.38	0.07	0.18	0.41
8	-0.08	0.08	0.00	0.16	0.16	0.69
14	0.12	0.15	-0.21	0.03	0.26	2.1
20	0.18	0.21	0.12	0.03	0.14	1.6
40	0.29	0.31	0.28	0.02	0.13	2.8
60	0.42	0.40	0.42	0.02	0.13	4.2
80	0.49	0.49	0.50	0.00	0.13	5.6
100	0.55	0.53	0.53	0.02	0.13	6.4

Data Point Summary - Indicator 1. - Service Port (lbf)

COMPRESSION

% of Range	Run 1 Error (%)	Run 2 Error (%)	Run 3 Error (%)	ASTM E4 Repeat Error (%)	Relative Uncertainty*	Uncertainty of Measurement* (± lbf)
100% Range (Full Scale: -4981.1 lbf)						
2	0.20	0.23	0.27	0.03	0.14	0.16
4	0.19	0.10	0.22	0.09	0.15	0.34
8	0.31	0.26	0.30	0.05	0.13	0.60
14	0.32	0.31	0.36	0.01	0.13	1.0
20	0.29	0.20	0.35	0.09	0.15	1.7
40	0.29	0.29	0.34	0.00	0.13	2.9
60	0.31	0.32	0.33	0.01	0.13	4.3
80	0.33	0.35	0.38	0.02	0.13	5.8
100	0.37	0.35	0.37	0.02	0.13	6.4

* The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

CERTIFICATE OF CALIBRATION

NVLAP ACCREDITED CALIBRATION LABORATORY No. 200301-0

CERTIFICATE NUMBER:

22082114091500

Page 3 of 5 pages

Data - Indicator 1. - Service Port (lbf)

TENSION

% of Range	Run 1		Run 2		Run 3	
	Indicated (lbf)	Applied (lbf)	Indicated (lbf)	Applied (lbf)	Indicated (lbf)	Applied (lbf)
100% Range (Full Scale: 4974.9 lbf)						
0 Return	0.160		-0.083		-0.073	
2	112.121	111.9768	115.867	115.7572	110.094	109.6316
4	223.598	223.236	218.340	217.8332	236.712	235.8096
8	426.810	427.15	465.843	465.45	429.701	429.7
14	803.277	802.3	796.953	795.75	781.594	783.25
20	1132.088	1130.05	1149.094	1146.7	1125.894	1124.5
40	2247.379	2240.85	2193.326	2186.65	2180.650	2174.65
60	3352.810	3338.9	3270.787	3257.7	3336.175	3322.15
80	4484.137	4462.2	4380.675	4359.2	4450.673	4428.6
100	4985.853	4958.35	5001.364	4974.9	4999.576	4973.2

Data - Indicator 1. - Service Port (lbf)

COMPRESSION

% of Range	Run 1		Run 2		Run 3	
	Indicated (lbf)	Applied (lbf)	Indicated (lbf)	Applied (lbf)	Indicated (lbf)	Applied (lbf)
100% Range (Full Scale: -4981.1 lbf)						
0 Return	0.048		0.049		0.178	
2	-119.086	-118.8512	-120.656	-120.3748	-115.443	-115.1332
4	-227.404	-226.98	-226.265	-226.0336	-230.006	-229.5072
8	-469.358	-467.9	-447.924	-446.75	-462.871	-461.5
14	-767.743	-765.3	-783.648	-781.25	-784.097	-781.25
20	-1131.395	-1128.1	-1136.474	-1134.25	-1141.256	-1137.25
40	-2231.311	-2224.75	-2144.291	-2138.05	-2235.596	-2228.05
60	-3344.884	-3334.65	-3362.566	-3351.95	-3343.339	-3332.4
80	-4403.484	-4389	-4451.333	-4435.85	-4449.687	-4432.7
100	-4991.488	-4973.15	-4998.538	-4981.1	-4999.734	-4981.5

The Return to Zero tolerance is \pm the indicator resolution, 0.1% of the maximum force verified in the range, or 1% of the lowest force verified in the range, whichever is greater.

CERTIFICATE OF CALIBRATION


NVLAP ACCREDITED CALIBRATION LABORATORY No. 200301-0

CERTIFICATE NUMBER:

22082114091500

Page 4 of 5 pages

Graphical Data - Indicator 1. - Service Port (lbf)

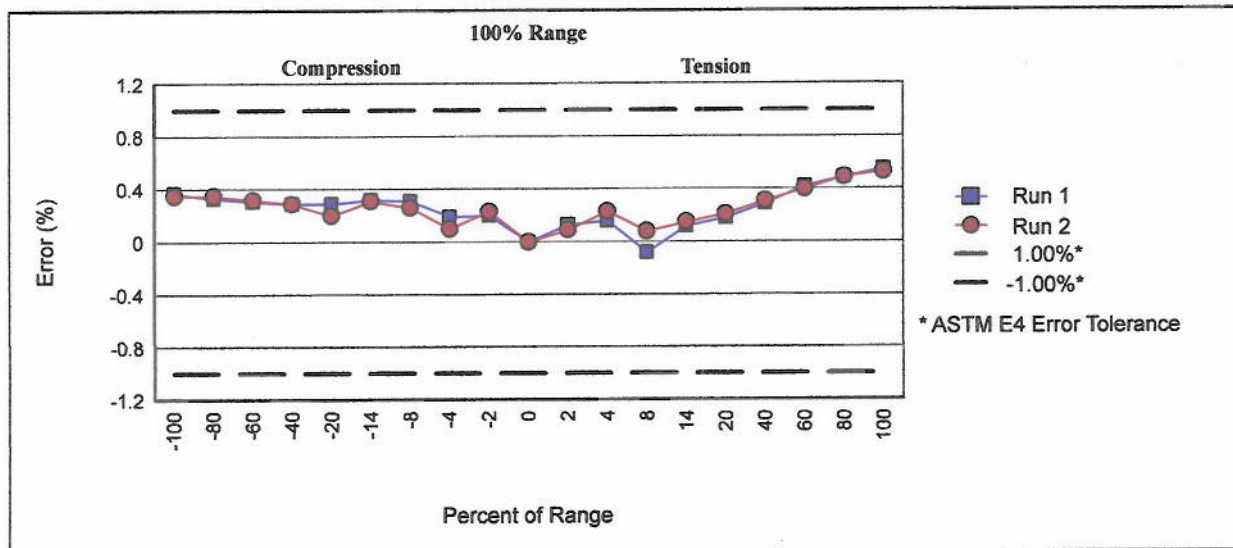

Verification Equipment

Make/Model	Serial Number	Description	Calibration Agency	Capacity	Cal Date	Cal Due
Exttech 445580	1001333	temp. indicator	Masy Systems Inc	NA	02-Oct-13	02-Oct-15
Flintec 10KFMM	198353	load cell	Instron	12000 lbf	16-May-14	16-May-16
Flintec 3401588	3401588	load cell	Instron	1200 lbf	31-Jan-14	31-Jan-16
HBM DK38	29480	force indicator	Instron	NA	23-Aug-12	23-Aug-14

Verification Equipment Usage

Range	Full Scale	Standard		Lower Limit for	
(%)	Mode	Serial Number	Percent(s) of Range	Standard (lbf)	Accuracy (+/-)
100	T	3401588	2/ 4	Class A1: 34	0.1% of reading
		198353	8/ 14/ 20/ 40/ 60/ 80/ 100	Class A1: 261	0.1% of reading
100	C	3401588	2/ 4	Class A1: 31	0.1% of reading
		198353	8/ 14/ 20/ 40/ 60/ 80/ 100	Class A1: 216	0.1% of reading
All	T/C	1001333	All	NA	2 °F

Instron standards are traceable to the SI (The International System of Units) through standards maintained by the National Institute of Standards and Technology (NIST) or other internationally recognized National Metrology Institutes (NMIs).

The standard Class A lower limit is used for systems with an accuracy of $\pm 1.0\%$ and the standard Class A1 lower limit is used for systems with an accuracy of $\pm 0.5\%$.

The accuracy of the force indicator used with elastic devices is incorporated into the devices stated accuracy.

Standard forces have been temperature compensated as necessary.

The accuracy of the verification equipment used was equal to or better than the accuracy indicated in the table above.

CERTIFICATE OF CALIBRATION

NVLAP ACCREDITED CALIBRATION LABORATORY No. 200301-0

CERTIFICATE NUMBER:

22082114091500

Page 5 of 5 pages

Comments

Verified by: Walt Szymanowski
Field Service Engineer

NOTE: Clause 19 of ASTM E4 states; It is recommended that testing machines be verified annually or more frequently if required. In no case shall the time interval between verifications exceed 18 months (except for machines in which long term test runs beyond the 18 month period). Testing machines shall be verified immediately after repairs that may in any way affect the operation of the weighing system or values displayed. Verification is required immediately after a testing machine is relocated and where there is a reason to doubt the accuracy of the force indicating system, regardless of the time interval since the last verification.